


## Chromatogram and Results

### Injection Details

Injection Name:	RTPT008 XR23101901-2	Run Time (min):	40.00
Vial Number:	G:A2	Injection Volume:	1.00
Injection Type:	Calibration Standard	Channel:	UV_VIS_1
Calibration Level:		Wavelength:	215
Instrument Method:	G2	Bandwidth:	n.a.
Processing Method:	醋酸处理办法	Dilution Factor:	1.0000
Injection Date/Time:	11/1月/24 13:24	Sample Weight:	1.0000

### Chromatogram

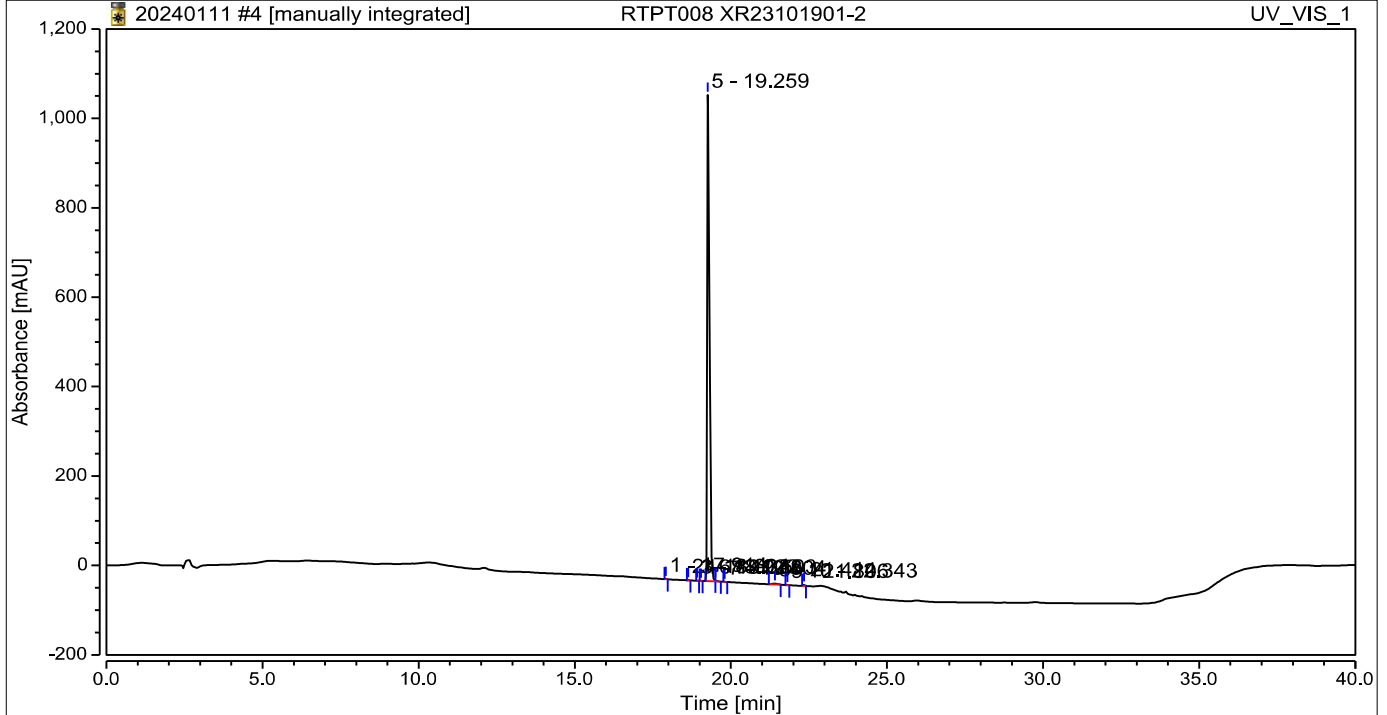

### Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount n.a.
1		17.914	0.0239	0.547	0.02	0.05	n.a.
2		18.634	0.0253	0.457	0.03	0.04	n.a.
3		18.923	0.0117	0.233	0.01	0.02	n.a.
4		19.038	0.0085	0.154	0.01	0.01	n.a.
5		19.259	95.5510	1087.901	99.18	99.18	n.a.
6		19.503	0.1046	1.802	0.11	0.16	n.a.
7		19.804	0.0118	0.200	0.01	0.02	n.a.
8		21.414	0.4087	2.304	0.42	0.21	n.a.
9		21.806	0.0201	0.346	0.02	0.03	n.a.
10		22.343	0.1740	2.986	0.18	0.27	n.a.
Total:			96.340	1096.931	100.000	100.000	