


Chromatogram and Results

Injection Details

Injection Name:	RTPT002 XR23110102-1-1	Run Time (min):	39.00
Vial Number:	R:A6	Injection Volume:	5.00
Injection Type:	Unknown	Channel:	UV_VIS_1
Calibration Level:		Wavelength:	215
Instrument Method:	SMLT-0.8ML标准方法	Bandwidth:	n.a.
Processing Method:	醋酸处理办法	Dilution Factor:	1.0000
Injection Date/Time:	22/4月/24 16:31	Sample Weight:	1.0000

Chromatogram

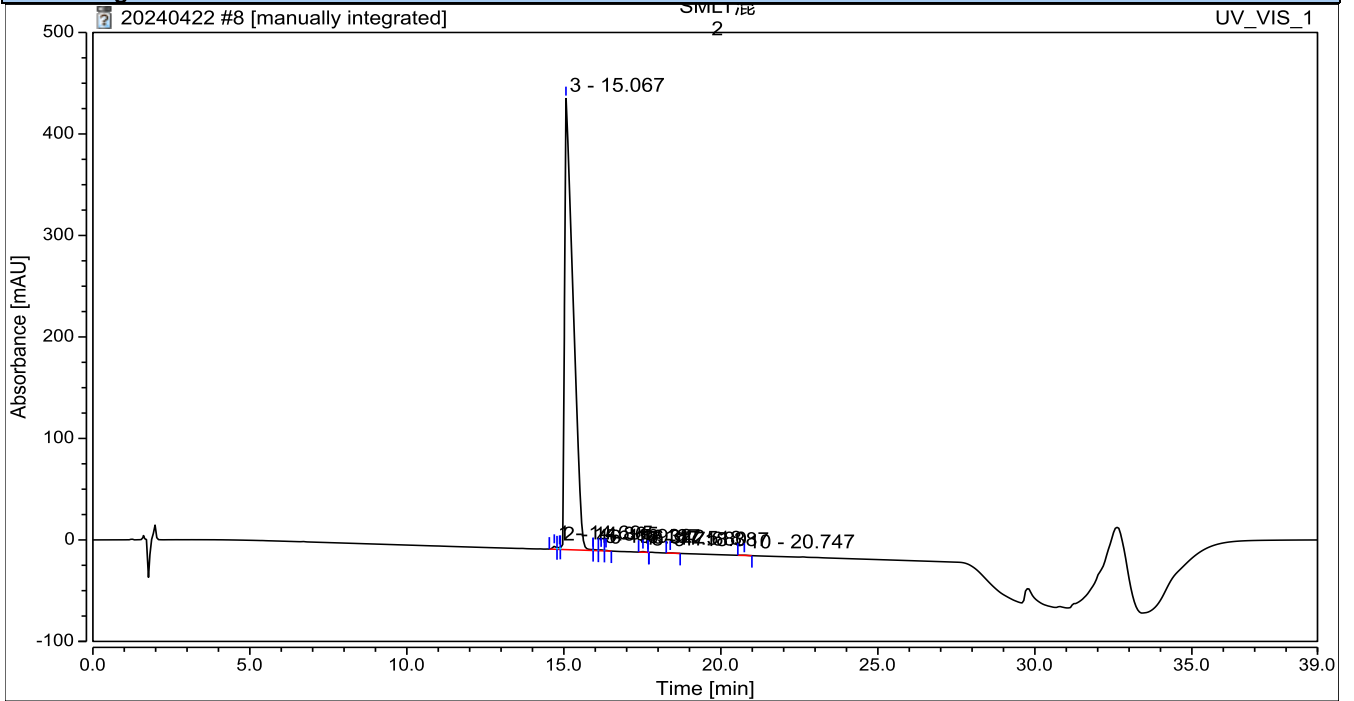

Integration Results

No.	Peakname	RetentionTime min	Area mAU*min	Height mAU	Relative Area %	Rel.Height %	Amount n.a.
1		14.695	0.3663	2.911	0.26	0.64	n.a.
2		14.865	0.1876	1.989	0.13	0.44	n.a.
3		15.067	139.1255	444.400	99.25	98.18	n.a.
4		15.932	0.1248	0.855	0.09	0.19	n.a.
5		16.187	0.1347	0.940	0.10	0.21	n.a.
6		16.342	0.0619	0.491	0.04	0.11	n.a.
7		17.518	0.0798	0.633	0.06	0.14	n.a.
8		17.680	0.0001	0.000	0.00	0.00	n.a.
9		18.387	0.0426	0.175	0.03	0.04	n.a.
10		20.747	0.0518	0.239	0.04	0.05	n.a.
Total:			140.175	452.633	100.000	100.000	